



Mechanical Circulatory Support LVAD, RVAD, and Bi-VAD

History

- SAMPLE
- Bridge to transplant
- Destination therapy
- Estimated downtime
- LVAD, RVAD, Bi-Vad, TAH
- DNR, MOST, or Living Will
- Contact with LVAD coordinator

Signs and Symptoms


- Unconsciousness
- Pulseless
- Apneic
- Poor capillary refill / skin color
- AMS or decreased mental status
- No electrical activity on ECG
- No heart tones on auscultation

Differential

- See Reversible Causes below
- Infection/Sepsis
- Hypovolemia
- Cardiac arrest
- Hemorrhage

Contact VAD coordinator:

- As quickly as possible for troubleshooting and treatment advice, but do not delay emergency treatment
- Follow patient specific emergency plan if present

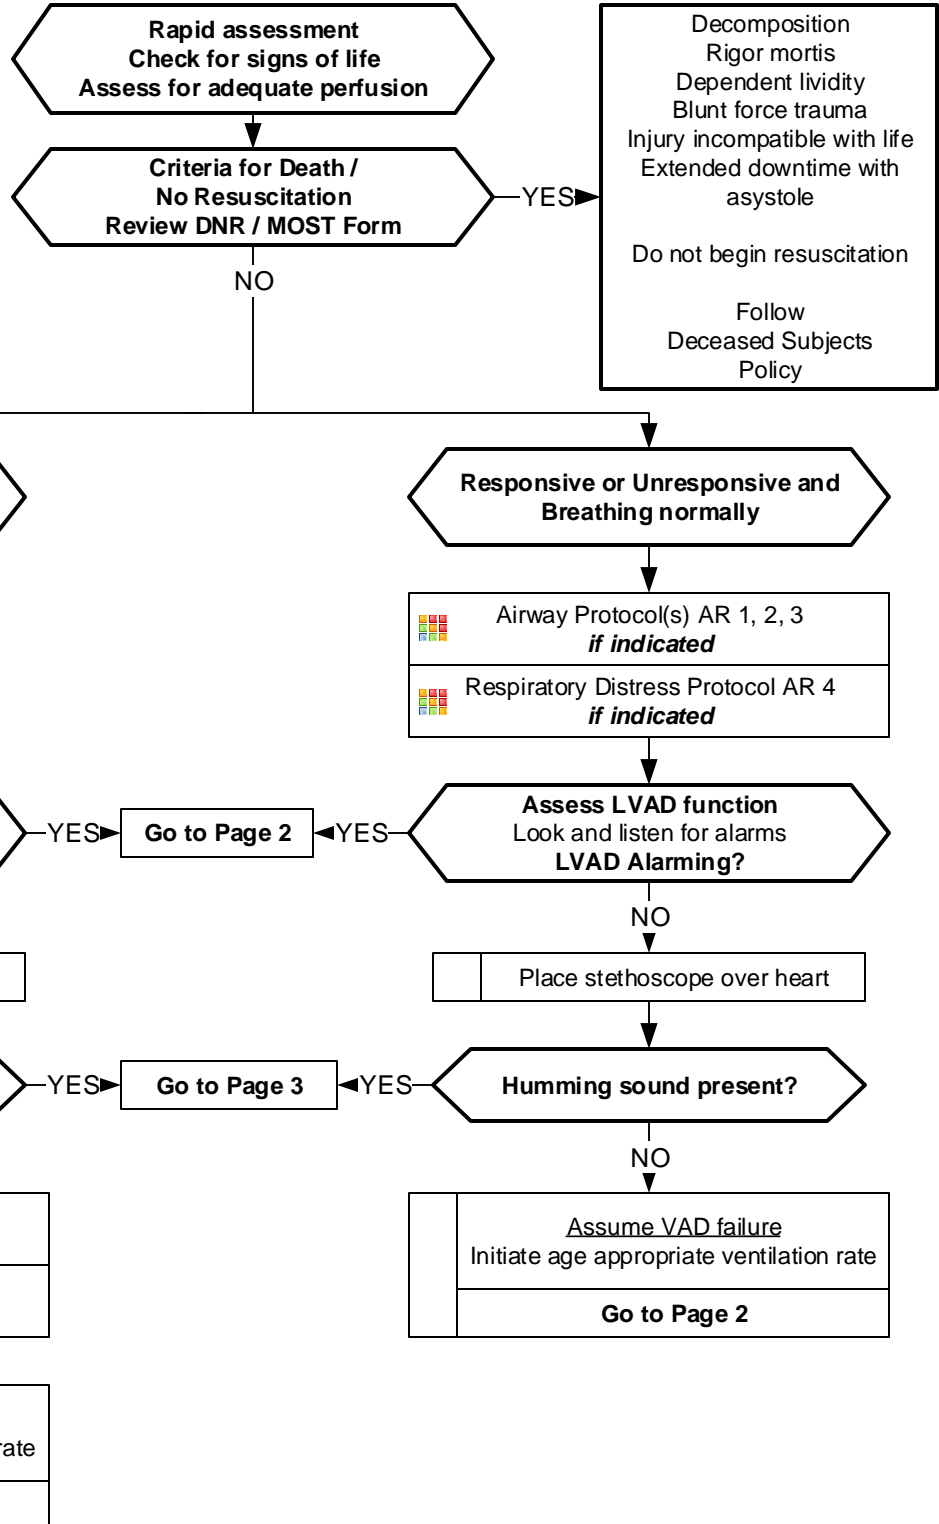

Adult Cardiac Protocol Section



Mechanical Circulatory Support LVAD, RVAD, and Bi-VAD

History


- SAMPLE
- Bridge to transplant
- Destination therapy
- Estimated downtime
- LVAD, RVAD, Bi-Vad, TAH
- DNR, MOST, or Living Will
- Contact with LVAD coordinator

Signs and Symptoms

- Unconsciousness
- Pulseless
- Apneic
- Poor capillary refill / skin color
- AMS or decreased mental status
- No electrical activity on ECG
- No heart tones on auscultation


Differential

- See Reversible Causes below
- Infection/Sepsis
- Hypovolemia
- Cardiac arrest
- Hemorrhage

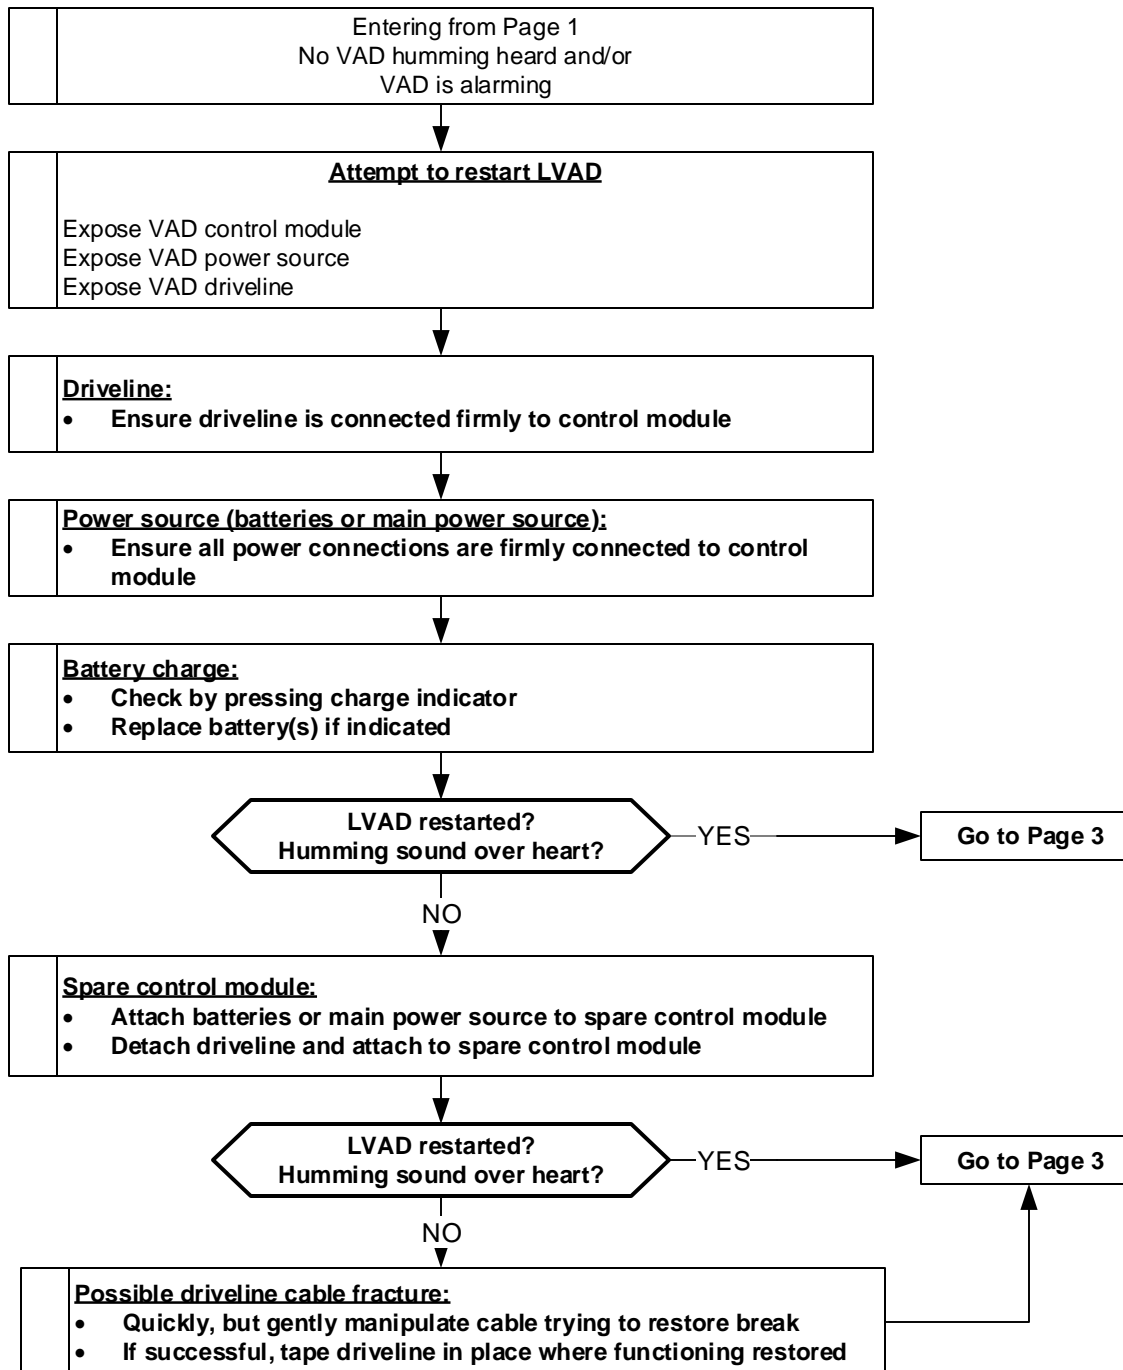



Mechanical Circulatory Support LVAD, RVAD, and Bi-VAD

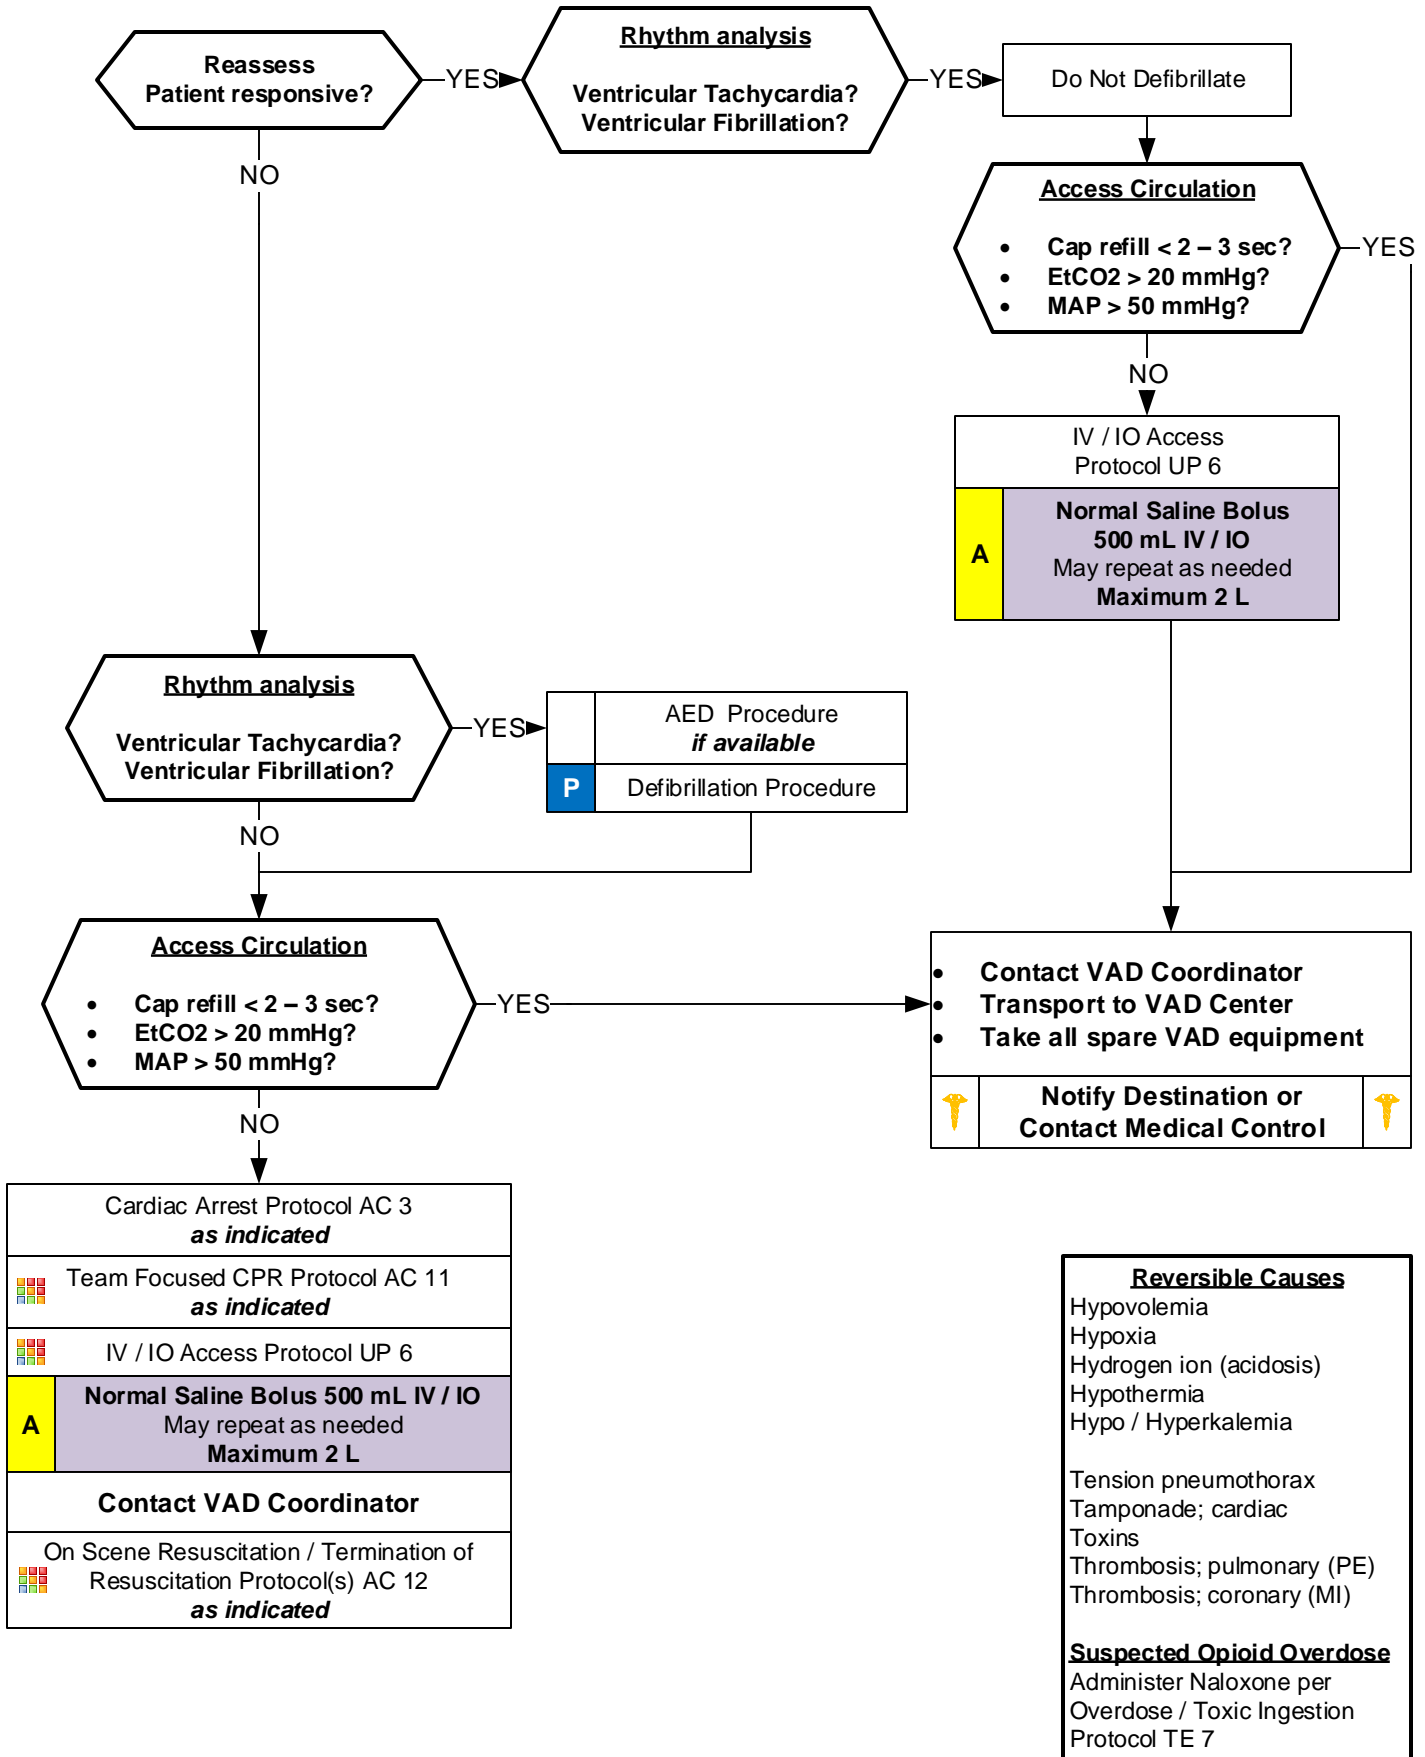



Left Ventricular Assist Device LVAD Unresponsive or AMS

Pearls

- **Recommended exam: Mental status, skin color, capillary refill, peripheral pulses, blood pressure.**
- **Assessment of blood flow and perfusion status:**
 - **Optimal BP attained by manual BP and Doppler.**
 - **Automated BP devices can measure a BP in about 50% of attempts and is not reliable to assess perfusion**
 - **A MAP of ≥ 60 mmHg is adequate for most LVAD patients.**
 - **Skin color, skin temperature, capillary refill**
- **Mechanical Circulatory Support devices:**
 - **LVAD – Left Ventricular Assist Device**
 - **RVAD – Right Ventricular Assist Device**
 - **BiVAD – Biventricular Ventricular Assist Device**
 - **TAH – Total Artificial Heart**
- **Reasons for use:**
 - **Bridge therapy – patients awaiting transplant or anticipated recovery.**
 - **Destination therapy – advanced heart failure, not candidate for transplant, and will live rest of life with device.**
- **Pump type and assessing pulses:**
 - **Pulsatile flow pumps – older units, not commonly in use now, but generate blood flow with a pulsatile flow and patient will have a palpable pulse.**
 - **Continuous flow pumps – majority of pumps now used and create blood flow in a continuous stream, no pulsatile flow, so patient will not have a palpable pulse.**
 - **Most devices are implanted inside the chest and have an internal pump, a driveline connected from the pump to the controller unit, and a power source consisting of batteries and electrical cord for receptacles.**
- **Common complications:**
 - **Disconnection of power supply, either battery disconnect, or electrical cord to receptacle disconnection.**
 - **Driveline failure or disconnection from controller unit.**
 - **Controller failure**
 - **Blood clot formation, acute stroke, and bleeding (mucosal and gastrointestinal most common sites)**
 - **Infection**
- **Abnormal heart rhythm:**
 - **Pseudo-PEA: Normal cardiac electrical activity in a patient who is alert and well perfused with no palpable pulse.**
 - **Tachyarrhythmias are usually well tolerated.**
- **End Tidal CO₂ (EtCO₂)**
 - **If EtCO₂ is < 10 mmHg, improve chest compressions. Goal is ≥ 20 mmHg.**
 - **If EtCO₂ spikes, typically > 40 mmHg, consider Return of Spontaneous Circulation (ROSC)**
- **Transcutaneous Pacing:**
 - **Pacing is NOT effective in cardiac arrest and pacing in cardiac arrest does NOT increase chance of survival**